

INSTRUCTIONS FOR USE AND HANDLING

RISPERDAL® ORAL SOLUTION

PRODUCT NAME

RISPERDAL® ORAL SOLUTION

(risperidone)

DOSAGE FORMS AND STRENGTHS

Oral Solution

The oral solution contains 1 mg/ml risperidone.

Always take this medicine exactly as your healthcare provider has told you. Check with your healthcare provider if you are not sure.

The solution comes with a syringe (pipette). Use only the syringe (pipette) delivered with this medicine for measuring the dose prescribed by your physician.




<p>Oral Solution</p> <p>Fig. 1: The bottle comes with a child-resistant cap and should be opened as follows:</p> <ul style="list-style-type: none"> - Push the plastic screw cap down while turning it counter clockwise. - Remove the unscrewed cap. 	<p style="text-align: center;">Dispensing Diagram</p> 
<p>Fig. 2: Insert the pipette into the bottle.</p>	

Fig. 3: While holding the bottom ring (Fig. 3a), pull the top ring up to the mark that corresponds to the number of milliliters or milligrams you need to give (See examples Fig. 3b).

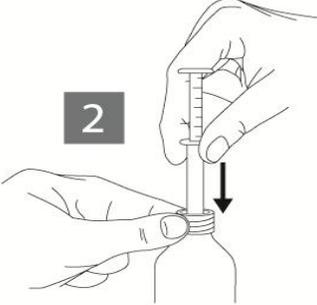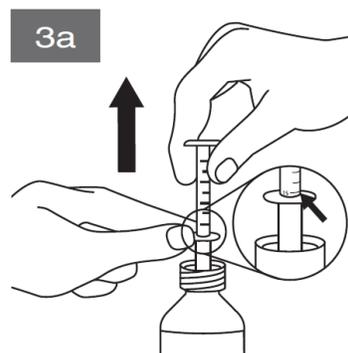

Measure the exact dose of medicine you need. Pay attention when measuring a small dose. For example, for 0.25 mg, measure 0.25 ml (a quarter milliliter); for 0.5 mg, measure 0.5 ml (half a milliliter).

1 ml of RISPERDAL oral solution contains 1 mg risperidone. The measured volume is printed every 0.25 ml / 0.25 mg on the plunger.

Fig. 3b shows **examples** of prescribed doses and corresponding marks on the plunger.


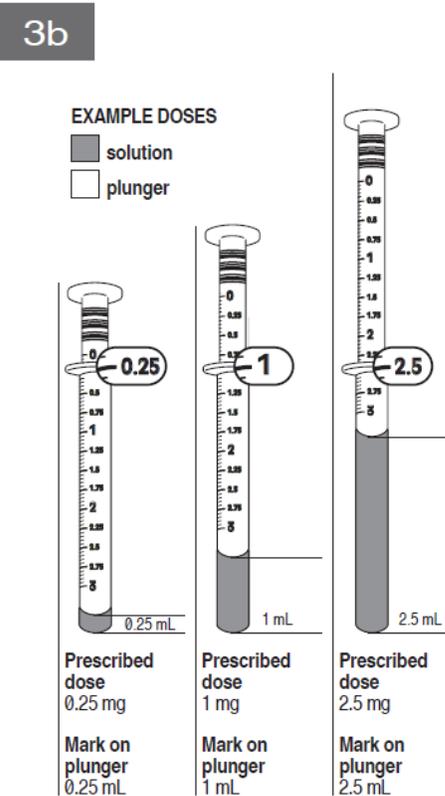


Fig. 4: Holding the bottom ring, remove the entire pipette from the bottle. Empty the pipette into any non-alcoholic drink, except for tea, by sliding the upper ring down. Close the bottle. Rinse the pipette with some water and let it air dry.

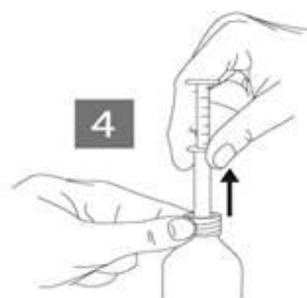

Marketing Authorization Number

1C 142/42(N)

Date of Authorization

Initial Authorization Date: 10 November 1999

DATE OF REVISION OF THE TEXT

CCDS version 04-Sep-2025

MANUFACTURED BY

Janssen Pharmaceutica N.V., Beerse, Belgium

Imported by

Janssen-Cilag Ltd., Bangkok, Thailand

To report Suspected Adverse Reactions, please contact us at aepqcjacth@its.jnj.com

For any product information, please contact us at medinfosea@its.jnj.com